
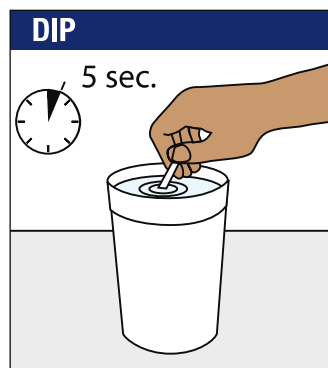


## TEST STRIP PROCEDURE


### 0.0 to 1.5 PPM CONCENTRATION RANGE

Tersano Stabilized Aqueous Ozone (SAO™) is approved to Standard AOAC 960.09 and ASTM E1153, for pre-cleaned use on hard, non-porous food prep and non-food prep surfaces as listed on product label.

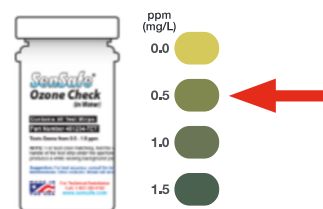


Dip one test strip into a 200mL room temperature water sample for 5 seconds with a constant, gentle back and forth motion (10 half strokes).

Remove the strip and shake once briskly, to remove excess water.

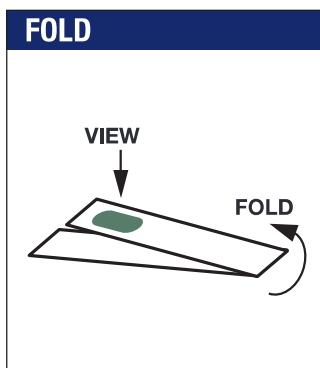

For best color matching, fold the white plastic handle of the test strip under the aperture so that it produces a white viewing background.

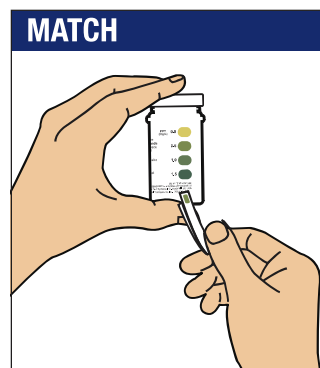

Match to the color chart at 30 seconds. Tersano SAO concentration is approved at **0.3ppm\***. A color match at 0.5ppm exceeds the approved sanitation range testing.

*\*ppm = parts per million*

### DIRECTION FOR USE

Apply SAO™ solution. Expose all surfaces to the sanitizing solution for a period of **not less than 30 seconds**. Air dry.



## Changing The Way The World Cleans